

GUARDIAN™ 4 TRANSMITTER



Medtronic

Medtronic, Medtronic with rising man logo, and Medtronic logo are trademarks of Medtronic. Third-party trademarks ("TM") belong to their respective owners. The following list includes trademarks or registered trademarks of a Medtronic entity in the United States and/or in other countries.

Guardian™, MiniMed™

Contacts:

Africa:

Medtronic South Africa and Southern Africa
Office Reception Tel: +27(0) 11 260 9300
Diabetes: 24/7 Helpline: 0800 633 7867
Sub-Sahara 24/7 Helpline: +27(0) 11 260 9490

Albania:

Net Electronics Albania
Tel: +355 697070121

Argentina:

Corpomedica S.A.
Tel: +(11) 4 814 1333
Medtronic Directo 24/7:
+0800 333 0752

Armenia:

Exiol LLC
Tel: +374 98 92 00 11
or +374 94 38 38 52

Australia:

Medtronic Australasia Pty. Ltd.
Tel: 1800 668 670

Bangladesh:

Sonargaon Healthcare Pvt Ltd.
Mobile: (+91)-9903995417
or (+880)-1714217131

Belarus:

Zarga Medica
Tel: +37517 336 97 00
+37529 613 08 08
+37517 215 02 89
Helpline: +74995830400

België/Belgique:

N.V. Medtronic Belgium S.A.
Tel: 0800-90805

Bosnia and Herzegovina:

"Novopharm" d.o.o. Sarajevo
Tel: +387 33 476 444
Helpline: 0800 222 33
Epsilon Research Intern. d.o.o.
Tel: +387 51 251 037
Helpline: 0800 222 33

Brasil:

Medtronic Comercial Ltda.
Tel: +(11) 2182-9200
Medtronic Directo 24/7:
+0800 773 9200

Bulgaria:

RSR EOOD
Tel: +359 888993083
Helpline: +359 884504344

Canada:

Medtronic Canada ULC
Tel: 1-800-284-4416 (toll free/sans-frais)

Česká republika:

Medtronic Czechia s.r.o.
Tel: +420 233 059 111
Non-stop helpLine (24/7):
+420 233 059 059
Zákaznický servis (8:00 - 17:00):
+420 233 059 950

Chile:

Medtronic Chile
Tel: +(9) 66 29 7126
Medtronic Directo 24/7:
+1 230 020 9750
Medtronic Directo 24/7 (From Santiago): +(2) 595 2942

China:

Medtronic (Shanghai) Management Co., Ltd.
Landline: +86 800-820-1981
Mobile Phone: +86 400-820-1981
Calling from outside China: +86 400-820-1981

Colombia:

Medtronic Latin America Inc. Sucursal Colombia
Tel: +(1) 742 7300
Medtronic Directo 24/7 (Landline):
+01 800 710 2170
Medtronic Directo 24/7 (Cellular):
+1 381 4902

Croatia:

Mediligo d.o.o.
Tel: +385 1 6454 295
Helpline: +385 1 4881144
Medtronic Adriatic d.o.o.
Helpline: +385 1 4881120

Danmark:

Medtronic Danmark A/S
Tel: +45 32 48 18 00

Deutschland:

Medtronic GmbH
Geschäftsbereich Diabetes
Telefon: +49 2159 8149-370
Telefax: +49 2159 8149-110
24-Stdn-Hotline: 0800 6464633

Eire:

Accu-Science LTD.
Tel: +353 45 433000

España:

Medtronic Ibérica S.A.
Tel: +34 91 625 05 42
Fax: +34 91 625 03 90
24 horas: +34 900 120 330

Estonia:

AB Medical Group Estonia Ltd
Tel: +372 6552310
Helpline: +372 5140694

Europe:

Medtronic Europe S.A. Europe, Middle East and Africa HQ
Tel: +41 (0) 21-802-7000

France:

Medtronic France S.A.S.
Tel: +33 (0) 1 55 38 17 00

Hellas:

Medtronic Hellas S.A.
Tel: +30 210677-9099

Hong Kong:

Medtronic Hong Kong Medical Ltd.
Tel: +852 2919-1300
To order supplies: +852 2919-1322
24-hour helpline: +852 2919-6441

India:

India Medtronic Pvt. Ltd.
Tel: (+91)-80-22112245 / 32972359
Mobile: (+91)-9611633007
Patient Care Helpline:
1800 209 6777

Indonesia:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Israel:

Medtronic Trading Ltd.
Tel.: +972-9-9724400
Tel. (product support –
8:00-17:00): +972-9-9724489
Helpline (weekends & holidays):
1-800-611-888

Italia:

Medtronic Italia S.p.A.
Tel: +39 02 24137 261
Fax: +39 02 24138 210
Servizio assistenza tecnica:
N° verde: 800 60 11 22

Japan:

Medtronic Japan Co. Ltd.
24 Hr. Support Line: 0120-56-32-56
日本：日本メドトロニック株式会社
24 時間サポートライン：
0120-56-32-56

Kazakhstan:

Medtronic BV in Kazakhstan
Tel: +7 727 311 05 80 (Almaty)
Tel: +7 717 224 48 11 (Astana)
Круглосуточная линия поддержки:
8 800 080 5001

Kosovo:

Yess Pharma
Tel: +377 44 999 900
Helpline: +37745888388

Latin America:

Medtronic, Inc.
Tel: 1(305) 500-9328
Fax: 1(786) 709-4244

Latvija:

RAL SIA
Tel: +371 67316372
Helpline (9am to 6pm):
+371 29611419

Lithuania:

Monameda UAB
Tel: +370 68405322
Helpline: +370 68494254

Macedonia:

Alkaloid Kons Dooel
Tel: +389 23204438

Magyarország:

Medtronic Hungária Kft.
Tel: +36 1 889 0688

Malaysia:

Medtronic International Ltd.
Tel: +603 7946 9000

México:

Tel (México DF): +(11) 029 058
Tel (Interior): +01 800 000 7867
Medtronic Directo 24/7 (from México
DF):
+(55) 36 869 787
Medtronic Directo 24/7:
+01 800 681 1845

Middle East and North Africa:

Regional Office
Tel: +961-1-370 670

Montenegro:

Glosarij d.o.o.
Tel: +382 20642495

Nederland, Luxemborg:

Medtronic B.V.
Tel: +31 (0) 45-566-8291
Gratis: 0800-3422338

New Zealand:

Medica Pacifica
Phone: 64 9 414 0318
Free Phone: 0800 106 100

Norge:

Medtronic Norge A/S
Tel: +47 67 10 32 00
Fax: +47 67 10 32 10

Österreich:

Medtronic Österreich GmbH
Tel: +43 (0) 1 240 44-0
24 – Stunden – Hotline: 0820 820 190

Philippines:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Россия

ООО «Медтроник»
Tel: +7 495 580 73 77
Круглосуточная линия поддержки
8 800 200 76 36

Polska:

Medtronic Poland Sp. z o.o.
Tel: +48 22 465 6934

Portugal:

Medtronic Portugal Lda
Tel: +351 21 7245100
Fax: +351 21 7245199

Puerto Rico:

Medtronic Puerto Rico
Tel: 787-753-5270

Republic of Korea:

Medtronic Korea, Co., Ltd.
Tel: +82.2.3404.3600

Romania:

Medtronic Romania S.R.L.
Tel: +40372188017
Helpline: +40 726677171

Schweiz:

Medtronic (Schweiz) AG
Tel: +41 (0)31 868 0160
24-Stunden-Hotline: 0800 633333
Fax Allgemein: +41 (0)318680199

Serbia:

Epsilon Research International d.o.o.
Tel: +381 113115554
Medtronic Serbia D.o.o
Helpline: +381 112095900

Singapore:

Medtronic International Ltd.
Tel: +65 6436 5090
or +65 6436 5000

Slovenija:

Zaloker & Zaloker d.o.o.
Tel: +386 1 542 51 11
24-urna tehnična pomoč:
+386 51316560

Slovenská republika:

Medtronic Slovakia, s.r.o.
Tel: +421 26820 6942
HelpLine: +421 26820 6986

Sri Lanka:

Swiss Biogenics Ltd.
Mobile: (+91)-9003077499
or (+94)-777256760

Suomi:

Medtronic Finland Oy
Tel: +358 20 7281 200
Help line: +358 400 100 313

Sverige:

Medtronic AB
Tel: +46 8 568 585 20
Fax: +46 8 568 585 11

Taiwan:

Medtronic (Taiwan) Ltd.
Tel: 02-21836000
Toll free: +886-800-005285

Thailand:

Medtronic (Thailand) Ltd.
Tel: +662 232 7400

Türkiye:

Medtronic Medikal Teknoloji
Ticaret Ltd. Sirketi.
Tel: +90 216 4694330

USA:

Medtronic Diabetes Global
Headquarters
24-Hour Technical
Support: +1-800-646-4633
To order supplies: +1-800-843-6687












Ukraine:













Med Ek Service TOV
Tel: +380 50 3311898
or +380 50 4344346
Лінія цілодобової підтримки:
0 800 508 300

United Kingdom:

Medtronic Ltd.
Tel: +44 1923-205167

Icon Table

	Serial number
	Catalogue number
(1x)	One per container/package
	Importer
	Medical device
	Date of manufacture
	Manufacturer
	Storage temperature limits
	Non-ionizing electromagnetic radiation
	Configuration or unique version identifier
	Type BF applied part
IP48	Transmitter: Protected against the effects of continuous immersion in water (2.4 meters (8 feet) immersion for 30 minutes).
	Storage humidity limits
CE0459	Conformité Européenne (European Conformity). This symbol means that the device fully complies with applicable European Union Acts.

	Fragile, handle with care
	Keep dry
	Recyclable, contains recycled content
	Do not dispose of this product in unsorted municipal waste stream
	Magnetic Resonance (MR) Unsafe
	Recharge-by date
	Bluetooth® wireless technology or Bluetooth® enabled
	Authorized representative in the European Community
	Complies with ANZ radiocommunications requirements
	Conformité Européenne (European Conformity). This symbol means that the device fully complies with applicable European Union Acts.
	Consult instructions for use
	Caution

Guardian 4

Introduction

The Guardian 4 transmitter (MMT-7841Q) with Bluetooth® wireless technology is a component of the continuous glucose monitoring (CGM) system with Bluetooth® wireless technology.

Indications for use

The Guardian 4 transmitter (MMT-7841Q) is a rechargeable device that powers the glucose sensor. The transmitter collects and calculates sensor data and sends the data via Bluetooth® wireless technology to a compatible display device, such as a mobile application, for the management of diabetes mellitus. The transmitter is only compatible with the Guardian 4 sensor (MMT-7040Q) and is indicated for single-patient or multiple-patient use. The transmitter is intended for persons ages 7 years and older.

Contraindications

No contraindications are associated with Guardian 4 transmitter use. For contraindications related to CGM, see the Guardian App User Guide.

Clinical Benefits

The Guardian 4 transmitter is a component of the CGM system that provides sensor glucose values. See the Guardian App User Guide for the clinical benefits of systems that use the Guardian 4 transmitter.

User Safety

Warnings

- Always refer to the Guardian 4 Sensor User Guide for all precautions, warnings, and instructions related to the sensor. Not referring to the Guardian 4 Sensor User Guide can result in serious injury or damage to the sensor.
- Do not allow children to put small parts in their mouth. This product may pose a choking hazard that can result in serious injury or death.
- Do not change or modify the device unless expressly approved by Medtronic Diabetes. Modifying the device can cause serious injury, interfere with the ability to operate the device, and void the warranty.
- Do not expose the transmitter to Magnetic Resonance Imaging (MRI) equipment, diathermy devices, or other devices that generate strong magnetic fields (for example x-ray, CT scan or other types of radiation). Exposure to a strong magnetic field has not been evaluated and can cause the device to malfunction, result in serious injury, or be unsafe. If the transmitter is exposed to a strong

magnetic field, discontinue use and contact a local Medtronic support representative for further assistance.

- Do not use the tester if it comes in contact with blood. Touching blood can cause infection.
- Bleeding may occur after inserting the sensor. Always make sure that the site is not bleeding before connecting the transmitter to the sensor. Blood can get into the transmitter connector and damage the device. Discard the device if damaged. If bleeding occurs, apply steady pressure with a sterile gauze, pad, or clean cloth at the insertion site until bleeding stops. After bleeding stops, connect the transmitter to the sensor.
- Do not discard the transmitter in a medical waste container or expose it to extreme heat. The transmitter contains a battery that may ignite and result in serious injury.
- If a serious incident related to the device occurs, immediately report the incident to a healthcare professional. For healthcare professionals, immediately report the incident to Medtronic and the applicable competent authority.
- For questions or concerns related to product use, contact a local Medtronic support representative for assistance.
- For medical questions or concerns, contact a healthcare provider.

Precautions


- Do not use the transmitter adjacent to other electrical equipment that may cause interference with the normal system operation.
- Only use the Guardian 4 sensor (MMT-7040Q) with the transmitter. Do not use any other sensor. Other sensors are not intended for use with the transmitter and will damage the transmitter and the sensor.
- Only use the green colored tester (MMT-7736L) with the transmitter. Do not use any other test plug. Other test plugs are not intended for use with the transmitter and will damage the transmitter and the tester.

Figure 1. Transmitter and tester



- Always use the tester when cleaning the transmitter. Do not use any other test plug with the transmitter. Use of another test plug can allow water to get into the transmitter or can prevent proper cleaning. Water can damage the transmitter.
- Do not twist the tester or sensor while attached to the transmitter. Twisting the tester or sensor will damage the transmitter.
- Do not allow the tester to come in contact with any liquid when not connected to the transmitter. A wet tester can damage the transmitter.
- Do not allow the transmitter to come in contact with any liquid when not connected to a sensor or to the tester. Moisture will damage the transmitter and a wet transmitter can damage the sensor.
- Do not clean the O-rings on the tester with any substances. Cleaning the O-rings can damage the tester.

Figure 2. O-rings

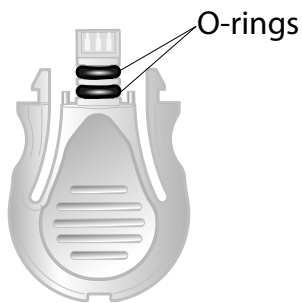

IEC 60601-1-2:2014, 4th Edition; Special EMC Precautions for Medical Electrical Equipment

1. Special Precautions regarding Electromagnetic Compatibility (EMC): This body worn device is intended to be operated within a reasonable residential, domestic, public or work environment where common levels of radiated “E” (V/m) or “H” fields (A/m) exist, such as cellular phones, Wi-Fi™, Bluetooth® wireless technology, electric can openers, microwave and induction ovens. This device generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the provided instructions, may cause harmful interference to radio communications.
2. Portable and mobile RF communications equipment can affect medical electrical equipment. If you encounter RF interference from a mobile or stationary RF transmitter, move away from the RF transmitter that is causing the interference.
3. Be careful when using the transmitter closer than 30 cm (12 in) to portable radio frequency (RF) equipment or electrical equipment. If the transmitter must be used next to portable RF equipment or electrical equipment, observe the transmitter to verify correct system operation. Degradation of the performance of the transmitter could result.
4. The essential performance (EP) of the transmitter is to measure and transmit to a monitoring device the sensing device’s signal value(s) within the transmitter’s accuracy requirements under the specified use conditions outlined in the Guardian App User Guide and for the duration of the expected service life. If the transmitter experiences electromagnetic disturbances, either no or incorrect data may be transmitted. In such situations, refer to the operation, maintenance, and troubleshooting instructions within the applicable user guides. You may also use the tester to test if the transmitter is operating properly. If the transmitter is damaged or if it cannot communicate with the display device, contact your local Medtronic support representative for assistance.

Assistance

Contact a local Medtronic support representative for assistance and if a copy of the Guardian App User Guide is needed.

Risks and side effects

The product contains small parts and may pose a choking hazard that can result in serious injury or death.

Side effects may include discomfort and skin irritation at the insertion site.

Hazardous substances

None.

Allergens


None known.

Using the transmitter

Components needed

- Guardian 4 transmitter (MMT-7841Q)
- Tester (MMT-7736L)
- Charger (MMT-7715)

Figure 3. Components

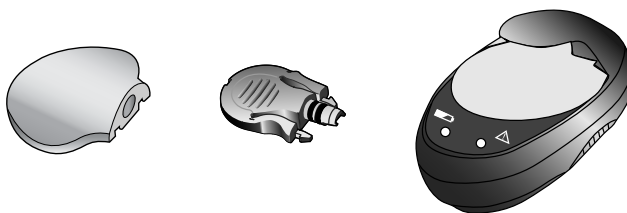

Preparing the transmitter


The transmitter contains a non-replaceable, rechargeable battery that can recharge as needed with the charger. The transmitter needs to be charged before use. The charger has a green light that shows the charging status and a red light that communicates any problems during charging. If there is a red light, see *Troubleshooting, page 29*. The charger requires one AAA alkaline battery.

Note: If the battery is installed incorrectly or is low, the charger will not work. Repeat the battery installation steps using a new battery.

Installing a battery in the charger

To install a battery in the charger:

1. Push the battery cover in and slide it off (as shown in image A in step 3).
2. Insert a new AAA alkaline battery. Make sure the + and - symbols on the battery align with these same symbols shown on the charger.
3. Slide the cover back on the charger until it clicks into place (as shown in image B in step 3).

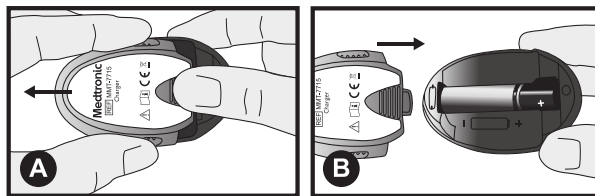


Charging the transmitter

CAUTION: Always charge the transmitter before inserting the sensor. A depleted transmitter does not function. A fully charged transmitter works at least seven days without recharging. A depleted transmitter can take up to two hours to recharge.


CAUTION: Do not store the transmitter on the charger for more than 60 days. Disconnect and reconnect to the charger to re-charge again before use. If the transmitter is left on the charger for more than 60 days, the transmitter battery will be permanently damaged.

To charge the transmitter:

1. Push the transmitter and the charger together to connect the transmitter to the charger.



2. Within 10 seconds after the transmitter is connected, a green light on the charger will flash for one to two seconds as the charger powers on. For the rest of the charging time, the green light on the charger will continue to flash in a pattern of four flashes with a pause between the four flashes.
3. When charging is complete, the green light on the charger will stay on, without flashing, for 15 to 20 seconds and then turn off.



4. After the green charger light turns off, disconnect the transmitter from the charger. The green light on the transmitter starts to flash.

Pairing the transmitter

The transmitter must be paired to the system before a sensor can be used. Always refer to the Guardian App User Guide for instructions on how to pair the transmitter to the system.

Inserting the sensor


Always refer to the Guardian 4 Sensor User Guide for instructions on how to insert the sensor.

Connecting the transmitter to the sensor


Before proceeding, have the Guardian App User Guide available.

To connect the transmitter to the sensor:

1. After the sensor is inserted, consult the Guardian 4 Sensor User Guide for details on how to apply the required tape before connecting the transmitter.
2. Hold the rounded end of the inserted sensor to prevent it from moving during connection.



3. Hold the transmitter as shown. Line up the two notches on the transmitter with the side arms of the sensor. The flat side of the transmitter should face the skin.



4. Slide the transmitter onto the sensor connector until the sensor arms snap into the notches on the transmitter. If the transmitter is properly connected, and if the sensor has had enough time to become hydrated with the interstitial fluid, the green light on the transmitter will flash 6 times.


Note: If the transmitter does not flash, see *Troubleshooting, page 29*.

5. When the transmitter light flashes green after connecting to the sensor, use the system to start the sensor. For more instructions, see the Guardian App User Guide.
6. Attach the adhesive tab of the sensor to the transmitter.
7. After the transmitter is connected, consult the Guardian 4 Sensor User Guide for instructions on how to apply a second tape.
8. Refer to the Guardian App User Guide for pairing.

Disconnecting the transmitter from the sensor

To disconnect the transmitter from the sensor:

1. Carefully remove any tape from the transmitter and sensor.



2. Remove the adhesive tab from the top of the transmitter.
3. Hold the transmitter as shown, and pinch the flexible side arms of the sensor between the thumb and forefinger.
4. Gently pull the transmitter away from the sensor.

Removing the sensor

Always refer to the Guardian 4 Sensor User Guide for instructions on how to remove the sensor.

Reconnecting the transmitter to a sensor that is already inserted

The transmitter can be reconnected to the sensor currently in use. Simply connect the transmitter to the sensor that is already inserted. Confirm Reconnect Sensor when the display device detects the transmitter. It may take a few seconds to establish a connection when reconnecting a sensor. Reattach the adhesive tab of the sensor to the transmitter and reapply any required tape. When reconnected, the sensor goes through another warm-up period.

Tester

The tester is used to test the transmitter to make sure it is working. The tester is also used as a required component to create a waterproof seal when cleaning the transmitter. Properly connecting the tester to the transmitter ensures that fluids do not come in contact with the connector pins inside the transmitter. Fluids can cause connector pins to corrode and affect the performance of the transmitter.

Do not twist the tester while attached to the transmitter. This will damage the transmitter.


The tester can be used for one year. If the tester is used for more than one year, the connector pins inside the transmitter can be damaged, because the tester cannot continue to provide a waterproof seal. For instructions on how to check the connector pins, see *Inspecting the transmitter connector pins*, page 18.

CAUTION: Only use the green colored tester (MMT-7736L) with the transmitter. Do not use any other test plug. Other test plugs are not intended for use with the transmitter and will damage the transmitter and the tester.



Inspecting the transmitter connector pins

This image is an example of how the connector pins should look for the transmitter.

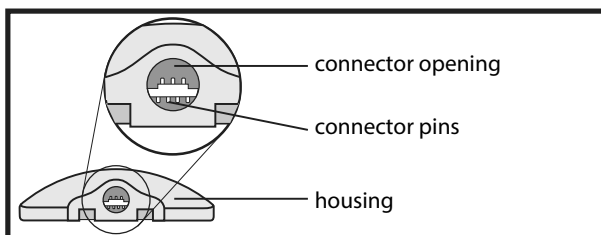

Look inside the connector opening of the transmitter to make sure that the connector pins are not damaged or corroded. If the connector pins are damaged or corroded, the transmitter cannot communicate with the charger or the display device. Contact a local Medtronic support representative. It may be time to replace your transmitter.


Look for moisture inside the connector opening. If any moisture is present, allow the transmitter to dry for at least one hour. Moisture inside the connector opening could cause the transmitter to not work properly and could cause corrosion and damage over time.

Connecting the tester for testing or cleaning

Before proceeding, have the Guardian App User Guide available.

To connect the tester:

1. Hold the transmitter body as shown and pinch the side arms of the tester.




2. Push the tester into the transmitter until the flexible side arms of the tester click into the notches on both sides of the transmitter.
When properly connected, the green light on the transmitter flashes 6 times.
3. To test the transmitter, check the sensor icon in the app to ensure that the transmitter is sending a signal (see the Guardian App User Guide).
4. To clean the transmitter, see *Cleaning the transmitter, page 20*.
5. After testing or cleaning, disconnect the tester from the transmitter.

Disconnecting the tester

To disconnect the tester:

1. Hold the transmitter body as shown and pinch the side arms of the tester.



2. With the tester arms pinched, gently pull the transmitter away from the tester.

Note: To save transmitter battery life, do NOT leave the tester connected after cleaning or testing.

Cleaning the transmitter

The transmitter is intended for personal use at home (single-patient use) or for use in healthcare facilities (multiple-patient use). Single-patient use requires cleaning after each use, while multiple-patient use requires cleaning and disinfection after each use. When using the transmitter in a healthcare facility, always follow the cleaning and disinfecting procedure for multiple-patient use.

WARNING: Do not discard the transmitter in a medical waste container or expose it to extreme heat. The transmitter contains a battery that may ignite and result in serious injury.

Note: The tester is a required component for cleaning the transmitter. For details, see *Tester*, page 17.

CAUTION: Do not use an automated washer-disinfector to clean or disinfect the device. Using an automated washer-disinfector to clean or disinfect the device will cause damage to the transmitter.

For single-patient use

Always clean the transmitter after each use.

To clean the transmitter, use these materials:

- mild liquid soap
- soft-bristled toddler toothbrush
- container
- clean, lint-free dry cloths


Use life

The transmitter can be cleaned up to 122 times or for one year, whichever comes first. Discard the transmitter at this point. If the transmitter is used beyond 122 times or one year, the cleaning process may damage the device. Contact a local Medtronic support representative to order a new transmitter.


WARNING: Do not use the device if there is any cracking, flaking, or damage to the housing. Cracking, flaking, or damage to the housing are signs of deterioration. Deterioration of the housing can affect the ability to properly clean the transmitter and result in serious injury. Call a local Medtronic support representative and discard the device according to local regulations for battery disposal (non-incineration), or contact a healthcare professional for disposal information.

To clean the transmitter:

1. Wash hands thoroughly.
2. Attach the tester to the transmitter to create a waterproof seal.




3. If there is adhesive residue on the transmitter, see *Removing adhesive residue*, page 28.
4. Rinse the transmitter under room temperature tap water for at least one minute, and until visibly clean. Make sure all hard-to-reach areas are rinsed completely.




5. Prepare a mild liquid soap solution using 5 mL (1 teaspoon) of mild liquid soap per 3.8 L (1 gallon) of room temperature tap water.


6. With the tester still attached, submerge the transmitter in the mild liquid soap solution and soak for one minute.




7. Holding the tester, brush the entire surface of the transmitter using a soft-bristled toddler toothbrush. Make sure to brush all hard-to-reach areas until visibly clean.




8. Rinse the transmitter under running room temperature tap water for at least one minute, and until all visible liquid soap is gone.



9. Dry the transmitter and tester with a clean, dry cloth.



10. Place the transmitter and tester on a clean, dry cloth and air dry them completely.
11. Disconnect the tester from the transmitter by gently squeezing the arms of the tester.



For multiple-patient use

When using the transmitter in a healthcare facility, always clean and disinfect the transmitter after each use.

WARNING: Standard precautions must be followed when handling or using this device. All parts of the system should be considered potentially infectious and are capable of transmitting blood-borne pathogens between patients and healthcare professionals.

The transmitter must be disinfected after use on each patient. This system may only be used for testing multiple patients when Standard Precautions and disinfection procedures provided by Medtronic Diabetes are followed.

To clean the transmitter, use these materials:

- gloves
- mild liquid soap

- soft-bristled toddler toothbrush
- 8.25% bleach
- two containers
- clean and lint-free dry cloths

Use life


The transmitter can be cleaned and disinfected up to 122 times or for one year, whichever comes first. Discard the transmitter at this point. If the transmitter is used beyond 122 times or one year, the cleaning and disinfection process may damage the device. Contact a local Medtronic support representative to order a new transmitter.

To clean and disinfect the transmitter:


1. Wash hands and put on gloves.
2. Inspect the inside of the transmitter's connector opening for any sign of body fluid. For instructions on how to inspect the connector pins, see *Inspecting the transmitter connector pins*, page 18.

CAUTION: The person inspecting the transmitter must have sufficient vision that enables him or her to see small drops of body fluid or debris.


WARNING: If there is any body fluid in the connector opening, the transmitter must be discarded. Because the transmitter contains a battery, do not discard in a bio-waste container. Instead, continue to clean and disinfect the transmitter, and then discard according to local regulations for battery disposal (non-incineration).

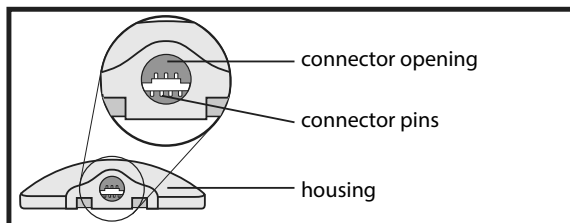


3. Attach the tester to the transmitter to create a waterproof seal.



4. If there is adhesive residue on the transmitter, see *Removing adhesive residue*, page 28.
5. Rinse the transmitter under room temperature tap water for at least one minute and until visibly clean. Make sure all hard-to-reach areas are rinsed completely.




6. Prepare a mild liquid soap solution using 5 mL (1 teaspoon) of mild liquid soap per 3.8 L (1 gallon) of room temperature tap water. Make sure to prepare a fresh solution for each use.
7. With the tester still attached, submerge the transmitter in the mild liquid soap solution and soak for one minute.




8. Holding the tester, brush the entire surface of the transmitter using a soft-bristled toddler toothbrush. Make sure to brush all hard-to-reach areas until visibly clean.




9. Rinse the transmitter under running room temperature tap water for at least one minute, and until all visible liquid soap is gone.




10. Dry the transmitter and tester with a clean, dry cloth.



11. Prepare a 1:10 bleach solution by using one (1) part 8.25% bleach to nine (9) parts water, for a final concentration of 0.8%. Make sure to prepare a fresh solution for each use.
12. Make sure that the previous cleaning steps are completed before disinfection. With the tester still attached, soak the transmitter in the bleach solution for 20 minutes.




13. Rinse the transmitter under running room temperature tap water for three minutes.



14. Place the transmitter and tester on a clean, dry cloth and air dry them completely.

WARNING: If there is any body fluid inside the connector opening on earlier inspection, the transmitter must be discarded with the tester still attached, according to local regulations for battery disposal (non-incineration).

15. Disconnect the tester from the transmitter by gently squeezing the arms of the tester.



16. Inspect the housing of the transmitter for any signs of cracking, flaking, or damage. If these signs are present, the transmitter must be discarded according to local regulations for battery disposal (non-incineration).

WARNING: Do not use the device if there is any cracking, flaking, or damage to the housing. Cracking, flaking, or damage to the housing are signs of deterioration. Deterioration of the housing can affect the ability to properly clean the transmitter, and result in serious injury. Call a local Medtronic support representative and discard the device according to local regulations for battery disposal (non-incineration), or contact a healthcare professional for disposal information.

17. Discard the used gloves and thoroughly wash hands with soap and water.

Removing adhesive residue


Follow these instructions if there is adhesive residue present on the transmitter.

Use cotton swabs and a medical adhesive remover such as Detachol™*, a mineral spirit, to remove adhesive residue.

Note: During testing, Detachol™* was used to remove the adhesive residue from the transmitter. Detachol™* is recommended for use but may not be available in all countries.

To remove adhesive residue:

1. Make sure the tester is attached to the transmitter.
2. Soak a cotton swab in the medical adhesive remover.
3. Hold the tester and gently rub the adhesive remover on the transmitter until the residue is removed.



4. Continue with the cleaning procedure. See *Cleaning the transmitter*, page 20 for details.

Cleaning the charger

This procedure is for general cleaning as required, based on physical appearance.

CAUTION: Do not immerse the charger in water or any other cleaning agent. The charger is not waterproof. Water can damage the charger and cause the device to malfunction.

To clean the charger:

1. Wash hands thoroughly.
2. Use a damp cloth with mild cleaning solution, such as a dishwashing detergent, to clean any dirt or foreign material from the outside of the charger. Never use organic solvents, such as paint thinner or acetone, to clean the charger.
3. Place the charger on a clean, dry cloth and air dry for two to three minutes.

Bathing and swimming

After the transmitter and sensor are connected, they form a waterproof seal to a depth of 2.4 meters (8 feet) for up to 30 minutes. Shower and swim without removing them.

Troubleshooting

The table shown contains troubleshooting information for the transmitter, charger, and tester. For more information about troubleshooting, see the Guardian App User Guide.

Table 1. Troubleshooting issues

Problem	Likely Cause(s)	Resolution
The transmitter is connected to the charger and no lights come on.	The transmitter connector pins are damaged or corroded. The charger battery has no power or no battery is inserted.	<ol style="list-style-type: none"> 1. Check the transmitter connector pins for damage or corrosion. For more information about the connector pins, see <i>Inspecting the transmitter connector pins, page 18</i>. If the pins are damaged or corroded, contact a local Medtronic support representative. It may be time to replace the transmitter. 2. If there is no damage to the connector pins, replace the battery in the charger. For instructions on replacing the charger battery, see <i>Installing a battery in the charger, page 13</i>.
During charging, the flashing green light on the charger turns off and a longer flashing red light appears on the charger.	The charger battery is low on power.	Replace the battery in the charger. For instructions on replacing the charger battery, see <i>Installing a battery in the charger, page 13</i> .
When charging, the flashing green light on the charger turns off and there is a series of quick flashing red lights on the charger for two seconds at a time.	The transmitter is low on power.	<ol style="list-style-type: none"> 1. Charge the transmitter continuously for one hour. If flashing does not stop, proceed to step 2. 2. Charge the transmitter continuously for eight hours. If flashing does not stop, call a local Medtronic support representative. It may be time to replace the transmitter.
During charging, a mix of quick and long flashing red lights appear on the charger.	The charger and the transmitter are low on power.	<ol style="list-style-type: none"> 1. Replace the battery in the charger. For instructions on replacing the charger battery, see <i>Installing a battery in the charger, page 13</i>. 2. Charge the transmitter continuously for one hour. If the quick flashing red lights do not stop, proceed to step 3. 3. Charge the transmitter continuously for eight hours. If flashing does not stop, call a local Medtronic support representative.

Table 1. Troubleshooting issues (continued)

Problem	Likely Cause(s)	Resolution
When connected to the sensor, the green light on the transmitter does not flash.	The transmitter is not fully connected. The transmitter is low on power. The sensor is not properly inserted into the body.	<p>tive. It may be time to replace the transmitter.</p> <ol style="list-style-type: none"> 1. Disconnect the transmitter from the sensor. 2. Wait for five seconds and reconnect them. If the green light still does not flash, proceed to step 3. 3. Fully charge the transmitter and connect it to the tester. If the green light still does not flash, see troubleshooting on "When connected to the tester, the green light on the transmitter does not flash." If the green light flashes, proceed to step 4. 4. Disconnect the transmitter from the tester, wait at least five seconds, and connect the transmitter to the sensor. If the green light still does not flash, proceed to step 5. 5. The sensor may not be properly inserted into the body. Remove the sensor from the body and insert a new sensor.
When connected to the tester, the green light on the transmitter does not flash.	The transmitter is not fully connected. The transmitter is low on power.	<ol style="list-style-type: none"> 1. Check the connection between the transmitter and the tester. If the green light still does not flash, proceed to step 2. 2. Fully charge the transmitter. 3. Test the transmitter with the tester again. If there is no flashing green light, call a local Medtronic support representative. It may be time to replace the transmitter.
The transmitter battery does not last for seven days.	The transmitter is not fully charged when connected to the sensor. The transmitter and display device frequently	<ol style="list-style-type: none"> 1. Fully charge the transmitter before connecting it to the sensor. If the transmitter battery still does not last for the duration of one sensor use, proceed to step 2. 2. Move away from any equipment that can cause RF interference. For more informa-

Table 1. Troubleshooting issues (continued)

Problem	Likely Cause(s)	Resolution
	lose wireless connection.	tion on RF interference, see the Radio Compliance Information sheet included with the display device. 3. Make sure the display device and the transmitter are located on the same side of the body to minimize any RF interference. If a fully charged transmitter battery continues to lose power before a full seven days, call a local Medtronic support representative. It may be time to replace the transmitter.
The transmitter loses connection with the display device.	The display device is out of range. There is RF interference from other devices.	1. Move away from any equipment that can cause RF interference. For more information on RF interference, see the Radio Compliance information sheet included with the transmitter. If the transmitter is still not communicating with the display device, proceed to step 2. 2. Make sure the display device and the transmitter are located on the same side of the body to minimize any RF interference. If the transmitter is still not communicating with the display device, call a local Medtronic support representative for assistance.
<p>Note: An alarm or alert occurs and a message appears when the transmitter has lost connection with the display device for 30 minutes.</p>		

Storage

Store the transmitter, charger, and tester in a clean, dry location at room temperature. If the transmitter is not in use, you must charge the transmitter at least once every 60 days.

CAUTION: Do not store the transmitter on the charger. If the transmitter is left on the charger for more than 60 days, the battery will be permanently damaged.

Disposal

Do not dispose of the transmitter, charger, and tester in unsorted municipal waste stream. Dispose of the transmitter, charger, and tester according to local regulations for electronic waste disposal.

Technical Specifications

Table 2. Product specifications

Biocompatibility	Transmitter: Complies with EN ISO 10993-1
Applied parts	Transmitter Sensor
Operating conditions	Transmitter temperature: 0°C to 45°C (32°F to 113°F) Caution: When operating the transmitter on a tester in air temperatures greater than 41°C (106°F), the temperature of the transmitter may exceed 43°C (109°F). Transmitter relative humidity: 10% to 95% with no condensation Transmitter pressure: 57.60 kPa to 106.17 kPa (8.4 psi to 15.4 psi) Charger temperature: 10°C to 40°C (50°F to 104°F) Charger relative humidity: 30% to 75% with no condensation
Storage conditions	Transmitter temperature: -20°C to 55°C (-4°F to 131°F) Transmitter relative humidity: up to 95% with no condensation Transmitter pressure: 57.6 kPa to 106 kPa (8.4 psi to 15.4 psi) Charger temperature: -10°C to 50°C (14°F to 122°F) Charger relative humidity: 10% to 95% with no condensation
Battery life	Transmitter: Seven days of continuous glucose monitoring immediately following a full charge. Charger: The charger uses one new AAA battery to charge the transmitter.
Transmitter frequency	2.4 GHz band, Bluetooth® wireless technology (version 4.0)
Effective radiated power (ERP)	-12.05 dBm (0.06 mW)
Effective isotropic radiated power (EIRP)	-9.9 dBm (0.1 mW)
Operating range	Up to 1.8 meters (6 feet) in free-air
Transmitter expected service life	The transmitter expected service life is one year depending on patient usage.

Transmitter wireless communication

Quality of service

The transmitter and display device connect via a Bluetooth® low-energy technology network. The transmitter sends glucose data and system-related alerts to the display device, which verifies the integrity of received data after wireless transmission. Quality of the connection is in accordance with the Bluetooth® Specification v4.0.

Data security

The transmitter is designed to only accept radio frequency (RF) communications from recognized and linked devices. The transmitter must be paired before the display device will accept information from the transmitter.

Display devices and system components (meters and transmitters) ensure data security via proprietary means and data integrity using error checking processes, such as cyclic redundancy checks.


Traveling by air

The transmitter is safe for use on commercial airlines. Because travel rules are subject to change, it is advisable to check with the Transportation Safety Administration (TSA) before traveling.

Guidance and manufacturer’s declaration

Guidance and Manufacturer’s Declaration - Electromagnetic Emissions		
Emissions Test	Compliance	Electromagnetic Environment - Guidance
RF emissions CISPR 11	CISPR 11 Group 1, Class B	The transmitter uses RF energy only for system communications. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment. Note: The preceding statement is required by IEC 60601-1-2 for Group 1, Class B devices. Since the transmitter is battery powered, its emissions will not be affected by the establishment power supply and there is no evidence of any issues associated with the use of the system in domestic establishments.
Harmonic emissions IEC 61000-3-2	Not applicable	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Not applicable	

Guidance and Manufacturer's Declaration - Electromagnetic Immunity			
Immunity Test	IEC 60601-1-2:2014 Test Level	Max foreseeable use condition per IEC 60601-1-2:2014	Electromagnetic Environment Guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air	±8 kV contact ±2 kV, ±4 kV, ±8 kV, ±15 kV air	For use in a typical domestic, commercial, or hospital environment.
Conducted disturbances induced by RF fields	3 V _{RMS} 150 kHz to 80 MHz 6 V _{RMS} ISM bands between 150 kHz to 80 MHz	Not applicable	Requirement does not apply to this battery powered device.
Electrical fast transient/burst IEC 61000-4-4	±2 kV 100 kHz repetition frequency	Not applicable	Requirement does not apply to this battery powered device.
Surge IEC 61000-4-5	Line to Line: ±0.5 kV, ±1 kV Line to Ground: ±0.5 kV, ±1 kV, ±2 kV	Not applicable	Requirement does not apply to this battery powered device.
Note: U _T is the a.c. mains voltage prior to application of the test level.			
Voltage dips, short interruptions, and voltage variations on power supply lines IEC 61000-4-11	0% U _T ; 0.5 cycles (at 0°, 45°, 90°, 135°, 180°, 225°, 270°, and 315°) 0% U _T ; 1 cycle (at 0°) 70% for 25/30 cycles (at 0°) 0% for 250/300 cycles	Not applicable	Requirement does not apply to this battery powered device.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	For use in a typical domestic, commercial, or hospital environment.
Proximity fields from RF wireless communications equipment IEC 61000-4-3	IEC 60601-1-2:2014, Table 9	IEC 60601-1-2:2014, Table 9	For use in a typical domestic, commercial, or hospital environment.
Note: U _T is the a.c. mains voltage prior to application of the test level.			
Radiated RF IEC 61000-4-3	10 V/m 80 MHz to 2.7 GHz	10 V/m 80 MHz to 6 GHz	Portable and mobile RF communications equipment

Guidance and Manufacturer's Declaration - Electromagnetic Immunity			
Immunity Test	IEC 60601-1-2:2014 Test Level	Max foreseeable use condition per IEC 60601-1-2:2014	Electromagnetic Environment Guidance
	80% AM at 1 kHz	80% AM at 1 kHz	<p>should be used no closer to any part of the transmitter than the recommended separation distance of 30 cm (12 in). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
<p>Note: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption, and reflection from structures, objects and people.</p>			

Warranty

Medtronic MiniMed, Inc. (or such other legal entity as may be referred to as manufacturer on the labeling of this device "Medtronic MiniMed") warrants the Medtronic transmitter to the purchaser of the product against defects in material and workmanship for a period of one (1) year and the charger for up to one (1) year from the date of purchase.

During the warranty period, Medtronic MiniMed will replace or repair, at its discretion, any defective transmitter or charger, subject to the conditions and exclusions stated herein. This warranty applies only to new devices. In the event a transmitter or charger is replaced, the warranty period will not be extended past its original expiration date.

This warranty is valid only if the Medtronic transmitter or charger is used in accordance with the manufacturer's instructions. Without limitation, this warranty will not apply:

- If damage results from changes or modifications made to the transmitter or charger by the user, or third persons, after the date of purchase.
- If damage results from service or repairs performed by any person or entity other than the manufacturer.
- If damage results from a *Force Majeure* or other event beyond the control of the manufacturer.
- If damage results from negligence or improper use, including but not limited to: improper storage, submersion in water, physical abuse, (such as dropping).
- If damage results from use of the device in a manner other than according to the manufacturer's product labeling, instructions for use, or regulatory notifications.

This warranty shall be personal to the original purchaser. Any sale, rental or other transfer or use of the product covered by this warranty to or by a user other than the original purchaser shall cause this warranty to immediately terminate. This warranty does not apply to glucose sensors and other accessories.

The remedies provided for in this warranty are the exclusive remedies available for any breach hereof. Neither Medtronic MiniMed nor its suppliers or distributors shall be liable for any incidental, consequential, or special damage of any nature or kind caused by or arising out of a defect in the product.

All other conditions and warranties, other than mandatory statutory warranties, expressed or implied, are excluded, including the warranties of merchantability and fitness for a particular purpose.

This warranty gives the purchaser specific legal rights, and the purchaser may also have other rights that vary under local law. This warranty does not affect the purchaser's statutory rights.

Open Source Software (OSS) Disclosure

This document identifies the Open Source Software that may be separately called, executed, linked, affiliated, or otherwise utilized by this product.

Such Open Source Software is licensed to users subject to the terms and conditions of the separate software license agreement for such Open Source Software.

Use of the Open Source Software by you shall be governed entirely by the terms and conditions of such license.

The source/object code and applicable license for the Open Source Software can be obtained at the following site: <http://www.ouah.org/ogay/hmac/>.

Medtronic



Medtronic MiniMed
18000 Devonshire Street
Northridge, CA 91325
USA
1 800 646 4633
+1 818 576 5555



Medtronic B.V.
Earl Bakkenstraat 10
6422 PJ Heerlen
The Netherlands

C €0459

© 2021 Medtronic
M811007A021_2
2021-03-23



MMT-7841Q, MMT-7920Q



M811007A021