



TRANSFER SETTINGS

MiniMed™ 630G pump to MiniMed™ 770G pump

STEP 1: Copy your current settings onto the Insulin Pump Settings Form. If for any reason you cannot copy the settings, please contact your healthcare professional.

STEP 2: Insert a AA battery into your new pump. You can use either a lithium, alkaline, or rechargeable battery.

STEP 3: Follow the instructions found in this guide to enter the settings that you have recorded on the Insulin Pump Settings Form into your new pump. For additional information on your pump, please consult the MiniMed™ 630G System User Guide.

Medtronic

We recommend that you record all settings on this form to refer to as you enter them into the new pump.

DELIVERY SETTINGS

BOLUS WIZARD SETUP

Menu > Options > Delivery Settings > Bolus Estimate Setup

Bolus Wizard: On Off

Carb Ratio:

12:00 A _____ g/U

_____ g/U

_____ g/U

Insulin Sensitivity Factor:

12:00 A _____ mmol/L per U

_____ mmol/L per U

_____ mmol/L per U

BG Target:

12:00 A _____ - _____ mmol/L

_____ - _____ mmol/L

_____ - _____ mmol/L

Active Insulin Time: _____ hr

BASAL PATTERN SETUP

Menu > Basal > Delivery Settings > Basal Pattern Setup

Basal 1:

12:00 A _____ U/hr Basal Pattern Name: _____

_____ U/hr 12:00 A _____ U/hr

_____ U/hr _____ U/hr

_____ U/hr _____ U/hr

PRESET TEMP SETUP

Menu > Options > Delivery Settings > Preset Temp Setup

Preset Temp Name: _____

Type _____ Percent _____ % Duration _____ hr

DUAL/SQUARE WAVE:

Menu > Options > Delivery Settings > Dual/Square Wave

Dual: On Off Square: On Off

PRESET BOLUS SETUP

Menu > Options > Delivery Settings > Preset Bolus Setup

Preset Bolus Name: _____

Bolus: _____ U Type: _____

% _____ Now _____ Square Duration _____ hr

DELIVERY SETTINGS (CONT.)

BOLUS INCREMENT:

Menu > Options > Delivery Settings > Bolus Increment

0.025U 0.05U 0.1U

MAX BASAL/BOLUS:

Menu > Options > Delivery Settings > Max Basal/Bolus

Max Basal: _____ U/hr Max Bolus: _____ U

EASY BOLUS:

Menu > Options > Delivery Settings > Easy Bolus

On Off Step Size _____ U

AUTO SUSPEND:

Menu > Options > Delivery Settings > Auto Suspend

On _____ hr Off

BOLUS SPEED:

Menu > Options > Delivery Settings > Bolus Speed

Standard Quick

UTILITIES

TURN SENSOR ON:

Menu > Options > Utilities > Sensor Settings

Sensor: On Off

DISPLAY OPTIONS:

Menu > Options > Utilities

Brightness _____ Auto Backlight _____ sec / min

SENSOR SETTINGS: HIGH SETUP Menu > Options > SmartGuard > High Setup

High Limit	Alert before high	Time before high	Alert on high	Rise Alert	Rise Limit*
12:00 A - _____ mmol/L	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mmol/L/min or ↑ ↑↑ ↑↑↑
_____ - _____ mmol/L	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mmol/L/min or ↑ ↑↑ ↑↑↑
_____ - _____ mmol/L	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mmol/L/min or ↑ ↑↑ ↑↑↑

SNOOZE Menu > Options > SmartGuard > Snooze > High Snooze: _____ hr

SENSOR SETTINGS: LOW SETTINGS Menu > Options > SmartGuard > Low Setup

Low Limit	Alert before low	Alert on low	Suspend on low
12:00 A - _____ mmol/L	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On
_____ - _____ mmol/L	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On
_____ - _____ mmol/L	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On

SNOOZE Menu > Options > SmartGuard > Snooze > Low Snooze: _____ hr

*Option only available when Rise Alert is on

STARTUP WIZARD

Once you've inserted the battery, the pump powers up and the **Startup Wizard** begins, it will guide you through setting language, time format, and current time and date.

1. Select **English**.
2. When the **Select Time Format** screen appears, select a **12 Hour** or a **24 Hour** time format.
3. When **Enter Time** screen appears, the hour will be flashing. Press **^** or **v** to the correct hour and press **O**.
4. The minutes will be flashing. Press **^** or **v** to the correct minutes and press **O**.
5. The **AM / PM** will be flashing. Press **^** or **v** if needed and press **O**. Select **Next**.
6. When the **Enter Date** screen appears, select **Year**. Press **^** or **v** to the correct year and press **O**. Repeat this step to set up **Month** and **Day**. Select **Next**.
7. The rewinding screen will briefly appear, followed by a confirmation message. Select **Ok**.



SETTING MAX BASAL

Menu > Options > Delivery Settings

1. Select **Max Basal/Bolus** and press **O**.
2. Select **Max Basal** to enter the **U/hr** amount. Use **^** and **v** to set the **Max Basal** amount. Press **O**.
3. Select **Save**.



SETTING MAX BOLUS

Menu > Options > Delivery Settings


1. Select **Max Basal/Bolus** and press **O**.
2. Select **Max Bolus** to enter the **U/hr** amount. Use **^** and **v** to set the **Max Bolus** amount. Press **O**.
3. Select **Save**.



SETTING BASAL PATTERN

Menu > Basal > Delivery Settings > Basal Pattern Setup

1. Select **Basal 1**.
2. Select **Options**, then select **Edit**.
3. Press **O** to enter **End** time. Press **O** to leave the **End** time at **12:00A**. If you are setting multiple rates use **^** or **v** to change the **End** time and press **O**.
4. Press **^** to enter **U/hr** and press **O**.
5. Continue adding **End** times and basal rates as needed, otherwise select **Done**.
6. Review the basal rates. If you need to correct, press **↶** to go back to edit mode. If Basal rates are correct select **Save**.







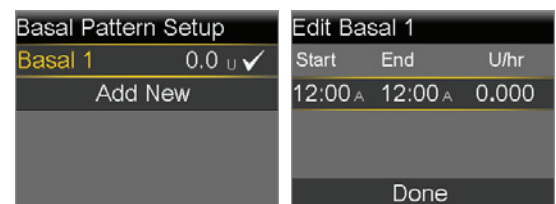


TURN BOLUS WIZARD ON AND SETUP

Menu > Options > Delivery Settings > Bolus Estimate Setup

1. Select **Bolus Wizard** to turn **On**.
2. Press **✓** to see the rest of the message then select **Next**.
3. Review the description of **Carb Ratio** and select **Next**.
4. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple Carb Ratios use **^** or **v** to change the **End** time, then press **○**.
5. Press **^** or **v** to enter g/U then press **○**.
Continue adding **End** times and **Carb Ratios** as needed.
6. Select **Next** when done.
7. Review the description of **Sensitivity Factor** and select **Next**.
8. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple **Sensitivity Factors**, use **^** or **v** to change the **End** time, then press **○**.
9. Press **^** or **v** to enter **mmol/L per U**, then press **○**.
Continue adding **End** times and **Sensitivity Factors** as needed.
10. Select **Next** when done.
11. Review the description of **BG Target** and select **Next**.
12. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple **BG Targets**, use **^** or **v** to change the **End** time, then press **○**.
13. Press **^** or **v** to enter **Lo** and then press **○**.
14. Press **^** or **v** to enter **Hi** and then press **○**.
Continue adding **End** times and **BG Targets** as needed.
15. Select **Next** when done.
16. Review the description of **Active Insulin Time** and select **Next**.
17. Press **○** to enter **Duration** time.
18. Press **^** or **v** to enter **hr** then press **○**.
19. Select **Save**.

The **Bolus Wizard** setup is now complete.

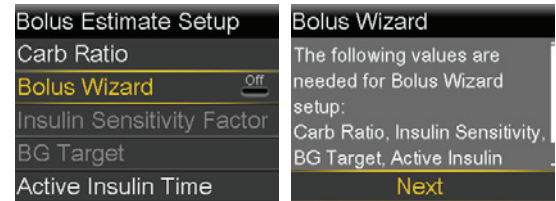


Note: The settings shown are for illustration purposes only — your settings may be different.

TURN SENSOR ON

Menu > Options > Utilities > Sensor Settings


1. Select **Sensor** to turn feature **On**.
You can now access the **SmartGuard** menu and enter the settings.

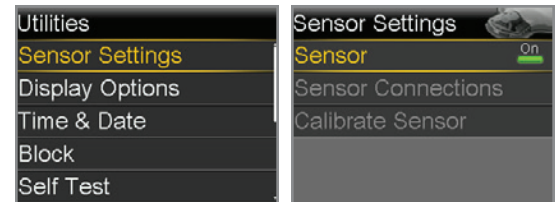

PROGRAMMING HIGH SETTINGS

Menu > Options > SmartGuard

1. Select **High Setup**.
2. Press **○** on the time segment. Press **○** again to leave the **End** time at **12:00A**. If setting multiple time segments, press **▲** to enter **End** time of first segment, and press **○**.
3. Press **▲** or **▼** to set **Hi** limit and press **○**. Press **○** to continue.
4. Select each feature you wish to turn on. If a feature is on, select it again to turn it back off.
5. Once settings are selected, select **Next** and then select **Done**.
6. Verify that settings are correct and select **Save**.
7. If snooze time needs to be changed, press **▼** to **Snooze** and press **○**.
Select **High Snooze**. Press **▲** or **▼** to enter the correct time and press **○**. Select **Save**.

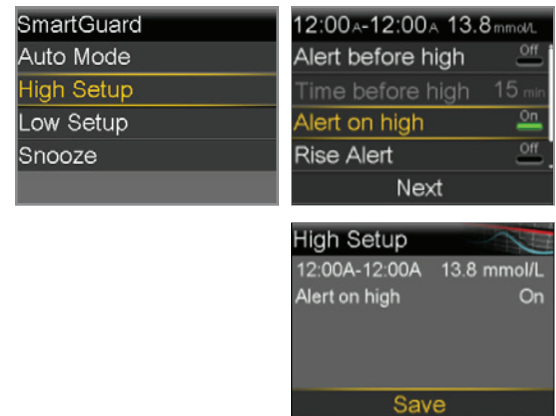


Your **High Setup** is now complete.

PROGRAMMING LOW SETTINGS

Menu > Options > SmartGuard

1. Select **Low Setup**.
2. Press **○** on the time segment. Press **○** again to leave the **End** time at **12:00A**. If setting multiple time segments, press **▲** to enter **End** time of first segment, and press **○**.
3. Press **▲** or **▼** to set **Lo** limit and press **○**. Press **○** to continue.
4. Select each feature you wish to turn on. If a feature is on, select it again to turn it back off.
5. Once settings are selected, select **Next** and then select **Done**.
6. Verify that settings are correct and select **Save**.
7. If snooze time needs to be changed, press **▼** to **Snooze** and press **○**.
Select **Low Snooze**. Press **▲** or **▼** to the correct time and press **○**. Select **Save**.

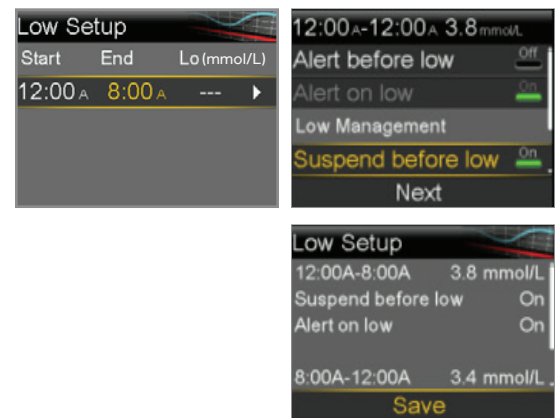

Your **Low Setup** is now complete.


Turn to page 5 to continue programming sensor settings.

TURN AUTO MODE ON

Menu > Options > SmartGuard

1. Select **Auto Mode**.
2. Select **Auto Mode** again to turn Auto Mode **On**.
3. Check the screen to make sure that Auto Mode is set to **On**.
Select **Save**


Note: If SmartGuard Auto Mode is not yet ready, after selecting **Save**, an alert occurs instructing to check the Auto Mode Readiness screen.


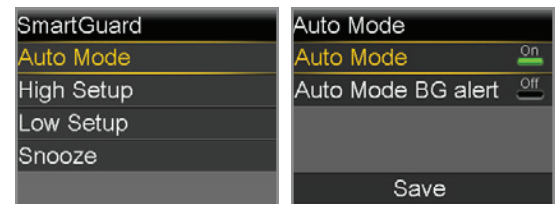


PAIR THE TRANSMITTER

Menu > Options > Utilities > Device Options > Pair Device

1. Attach your transmitter to the charger and place next to the pump.
2. Select **Search** on the pump and immediately remove the transmitter from the charger.
3. The **Select Device** screen appears with a list of available devices. Select the **CGM** device that matches the serial number (**SN**) on your transmitter.
4. Make sure the serial number on the pump screen and transmitter match and select **Confirm**.

Your pump displays a message if the pump and transmitter are paired successfully. If the Sensor feature is turned on, the Connection icon  appears on the Home screen.

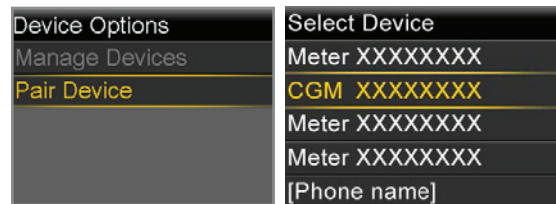

Please take some time to review ALL your entries and ensure they are correct.

In Need of Technical Assistance?

24-Hour Technical Support Is Here to Help

Call 1-800-284-4416

For medical advice, contact your healthcare team.

Note: If you turn Auto Mode on before the 48 hour warm up is complete, you may receive an alert at midnight to Enter a BG for Auto Mode. To avoid this, you may want to wait to turn on Auto Mode on day 3 of your pump wear.